



## Changing the Next Technical Safety Check Date on an Erbe VIO® 3 Electrosurgical Unit

- Power on the unit and access the Main Menu
- Select “**Service**” in the bottom left corner as indicated below.

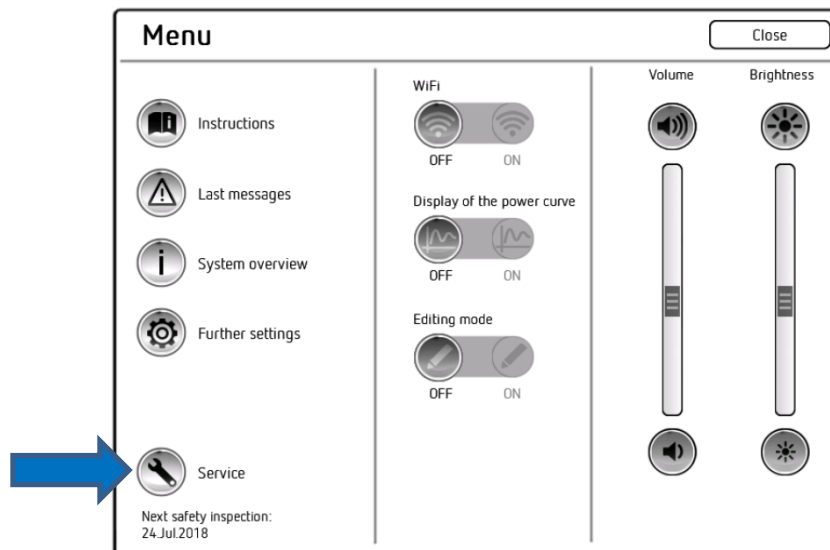

- Input the password; “VIO3”, then press “Enter”.
- Select “**Next technical safety check**”.

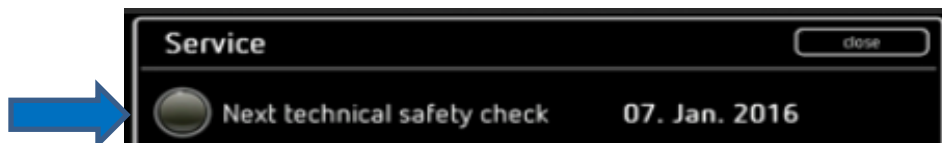

- Select “**Set next technical safety check to:**”
- The date will advance to one year ahead of the current date.

If you have any concerns or questions, please call the Technical Service staff at 800-778-3723.